


EM=330

LCMS Scan ESI-

Ret. Time: 3. 59 <<< NEGATIVE SPECTRA >>>

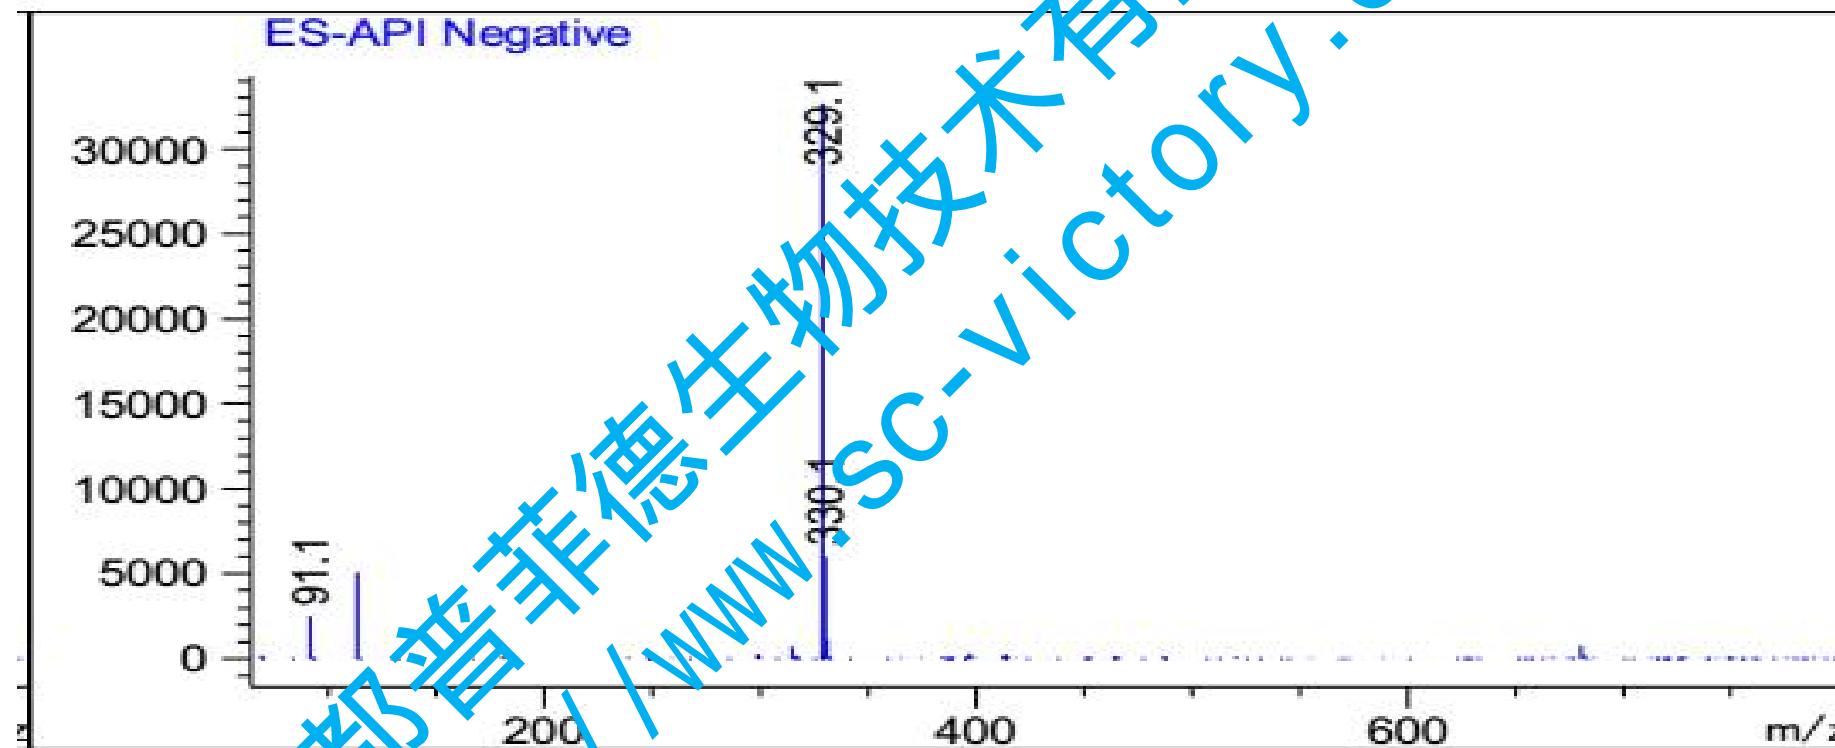

成都唯德生物技术有限公司
http://www.sc-victory.com